

# CONCISE SEPARATIONS


## Coregel 64H

P/N: ICE-99-9860

Processing Method: 64H  
Sample Name: Test Mixture  
High Selectivity  
Column S/N: 12911928

Volume: 20 uL  
Length: 300 mm  
ID: 7.8 mm  
Polymer Lot: 123-120

UV 210nm

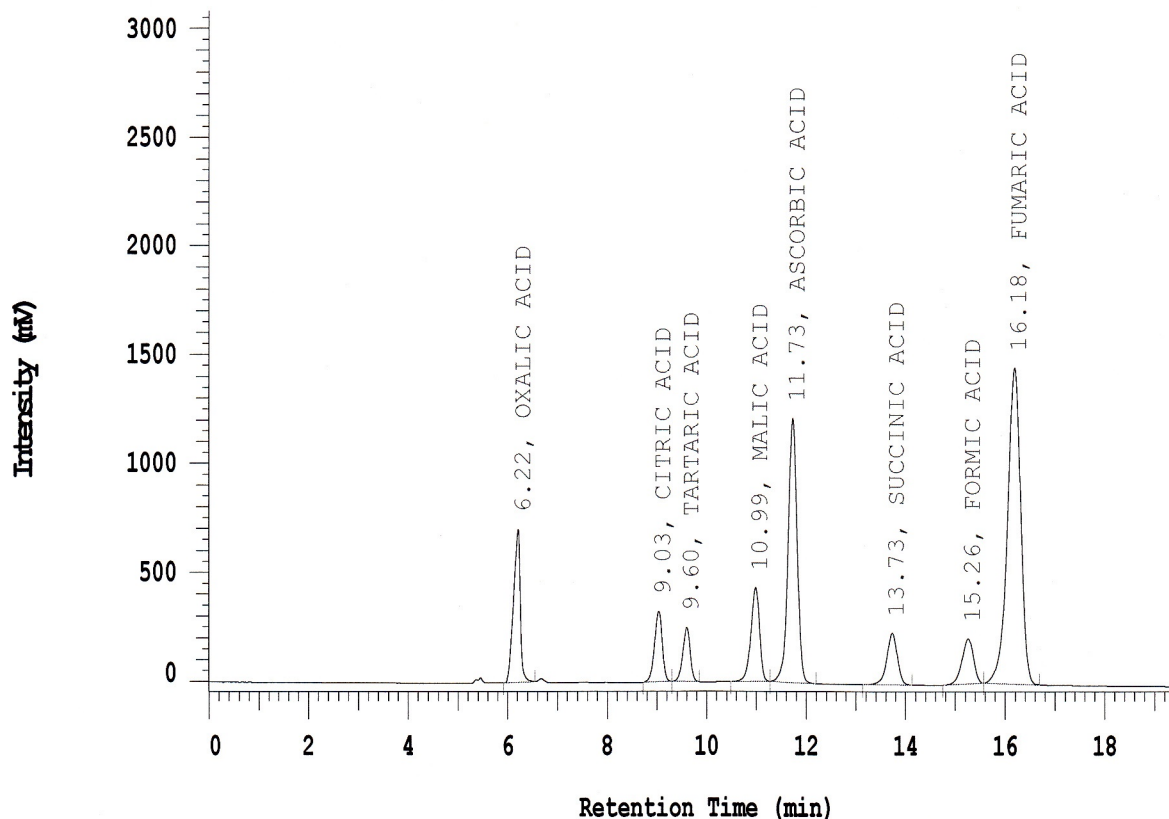

System 3

Solvent: 0.008N H2SO4

Flow Rate: 0.6 ml/min

Temperature: 50C

Pump A Pressure Profile: Max: 768.2 Min: 754.0

RT (min)	Name	k'	Asym	N (EUP)	Res (EUP)	Alpha	S/N	Noise (uV)
6.22	OXALIC ACID	620.67	0.80	10636	---	---	---	---
9.03	CITRIC ACID	902.33	0.92	16945	10.86	1.45	---	---
9.60	TARTARIC ACID	959.00	0.89	19737	2.06	1.06	---	---
10.99	MALIC ACID	1097.67	0.87	19895	4.74	1.14	---	---
11.73	ASCORBIC ACID	1171.67	0.93	21289	2.34	1.07	---	---
13.73	SUCCINIC ACID	1371.67	0.91	20317	5.66	1.17	---	---
15.26	FORMIC ACID	1525.00	0.91	20710	3.79	1.11	---	---
16.18	FUMARIC ACID	1617.00	0.89	18749	2.05	1.06	---	---

